



Carlton System

Surgical Technique

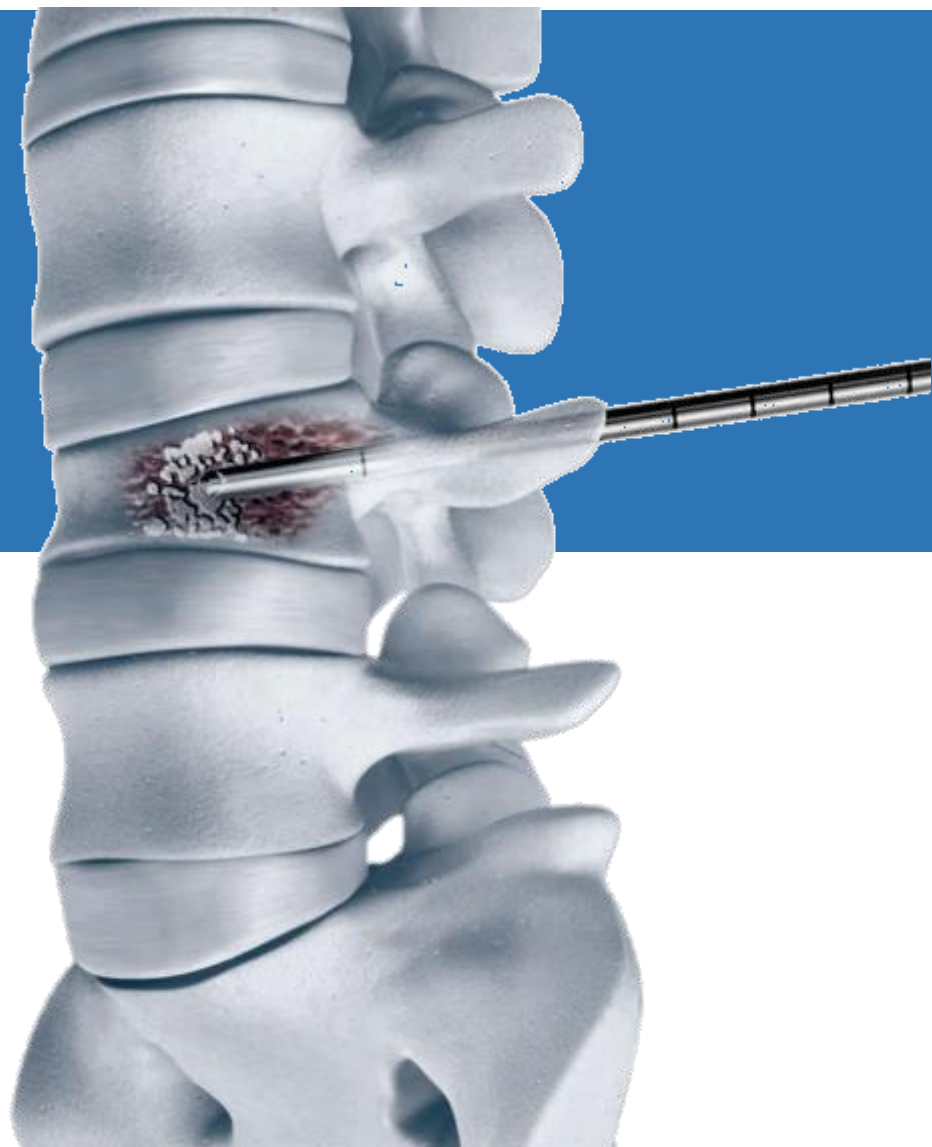


Pump

- The cylinder needle has a pressure gauge that can be shown on the LCD screen to indicate the capacity used to restore the spinal bone. Maximum allowable level of 300psi applies.
- There is an adjustment to increase or decrease the lock application.
- The processor applies a new stable and accurate processing method.
- There is a measuring scale to help reserve the required amount of cement with vivid quality into the body.
- Compact and some simple components in the kit.
- Easy to use.

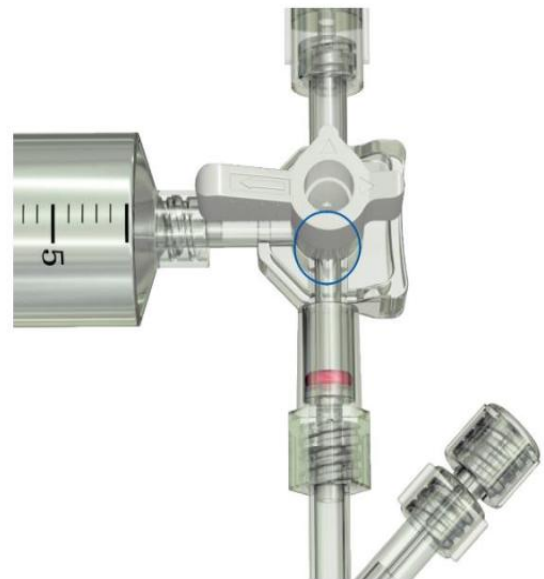


Pump

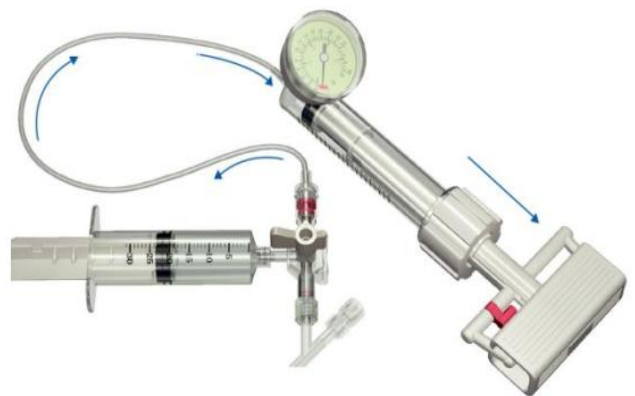

Product Code

S771762000

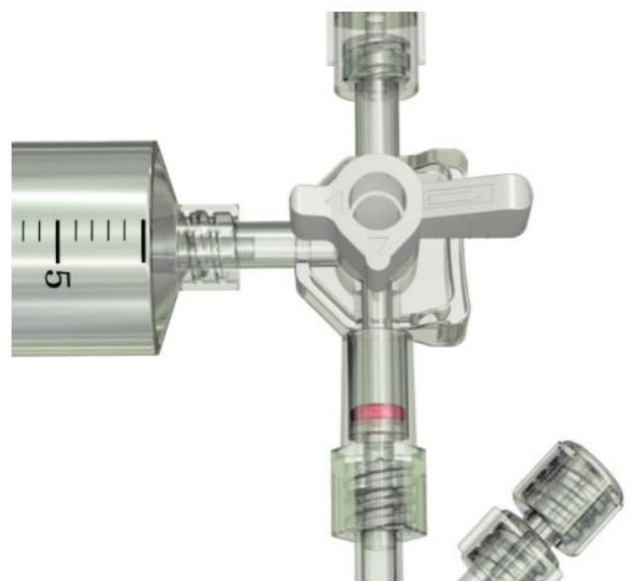

Mixing Set

Mixing capacity 40ml.
 Closed System mixing device.
 Funnel and spatula included.
 Includes 4 5ml syringes.



Trocar

- Materials: Medical alloy, beveled needle, T-handle and barrel (trocar).
- Dimensions: 3.0 x 120mm.
- Used to penetrate the hard bone shell of the small pedicle of the damaged vertebra.
- Detect photosensitivity on the needle body when taking X-rays.
- Standards for subcutaneous vertebrae procedures.
- The bevel angle is designed to easily penetrate through the bone cortex.
- Lockable chuck handle.
- A laser mark allows control of penetration depth.
- Used with shineless cement pumping system.



Trocar



B

Specification	Product Code
φ3.0 x 120, G11	S771760211
φ3.0 x 120, G13	S771760213

PKP Kit (No Balloon) (S771760000)

Product Code	Product Name	Specification	Quantity	Picture
S771760211	Trocar	3.0*120	/	
S771760213	Trocar	3.0*120	/	
S771762000	Pump	/	/	